


TML\MSH Microbiology Department Policy & Procedure Manual	Policy # MI/SER/17/06/v01	Page 1 of 1
Section: Serology Manual	Subject Title: Appendix VI BDProbeTec ET Workflow	
Issued by: LABORATORY MANAGER	Original Date: May 26, 2003	
Approved by: Laboratory Director	Revision Date:	

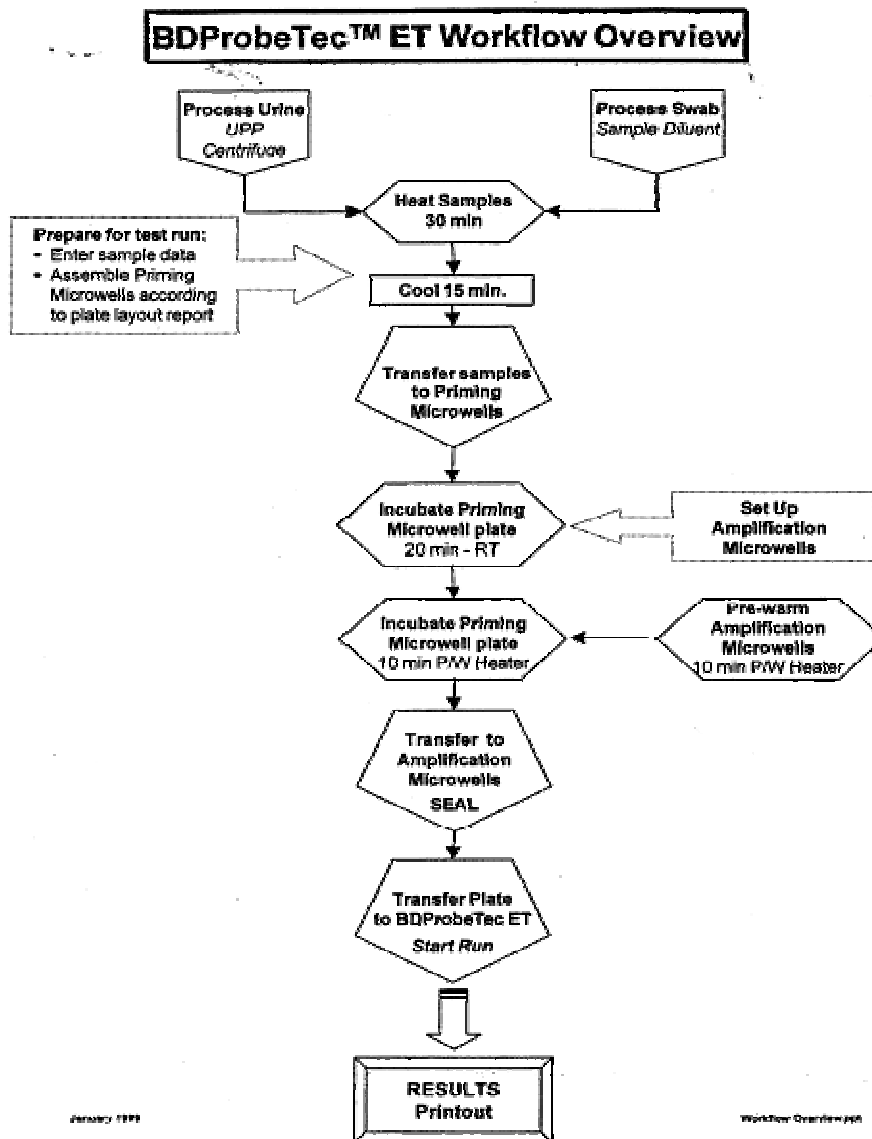

← Processed swabs good for:

- 6 hrs at RT
- Overnight at 4 C

← Cooled samples good for :

- 6 hrs at RT
- 5 days at 4 C, then re-lysed
- 98 days frozen (-20 C), then re-lysed

Good for 6 hrs at RT →